

CHEMSCAN UV-SERIES ANALYZERS GRAPHIC USER INTERFACE

USER GUIDE



Contact your ChemScan Regional Manager for additional information
on the ChemScan UV-Series Analyzer

1 Contents

1.	Safety	4
2.	Analyzer Description	5
2.1.	Analyzer Analysis Modes	5
2.1.1.	Flush Cycle.....	5
2.1.2.	Scanning Sample	5
2.1.3.	Reagent Addition	5
2.1.4.	Mixing Sample.....	5
2.1.5.	Idle or Reacting	5
3.	Operation	6
3.1.	HMI Definition.....	6
3.1.1.	HMI Components	6
3.2.	Home Screen.....	6
3.2.1.	Home Screen – Top Level Buttons	7
3.2.2.	Home Screen – Parameter and Operation Groups	8
3.3.	Main Screen	8
3.3.1.	Initiate On-Line Mode	9
3.3.2.	Exit On-Line Mode.....	9
3.3.3.	Navigation Short Cuts	10
3.3.4.	Parameter Screen Group	10
3.3.4.1.	Parameter View Screen (On-Line Mode)	11
3.3.4.2.	Parameter View Screen (Off-Line Mode).....	11
3.3.4.3.	Parameter Settings Screen (Off-Line Mode)	12
3.3.4.4.	Parameter Manual Read Screen (Off-Line Mode)	12
3.3.4.5.	Data log Retrieval Screen.....	13
3.4.	Operational Screen	14
3.4.1.	Analyzer Function Screen (On-Line Mode)	14
3.4.2.	Analyzer Function Screen (Off-Line Mode).....	15
3.4.3.	Manual Component Operation.....	15
3.4.4.	Analyzer Operation Group	15
3.4.4.1.	Manual Zero Screen	16
3.4.4.2.	Prime Injectors Screen	16
3.4.4.3.	Operational Settings	17

3.4.4.4.	Sample Line Settings	17
3.4.4.5.	Zero Settings	18
3.4.4.6.	Memory Backup	18
3.4.4.7.	Memory Restore	19
3.4.4.8.	Clock and Screen Settings	19
3.4.4.9.	Password Settings	19
3.4.5.	Warnings and Errors –.....	20
3.4.6.	Help	20
4.	Maintenance	21
4.1.	Manual Analyzer Zeroing Procedure	21
4.1.1.	Interrupt on-line mode:	21
4.1.2.	Analyzer Operation Screen	21
4.1.3.	Analyzer Zero Screen – Reading the Zero	22
4.1.4.	Analyzer Zero Screen – Testing the Zero	22
4.1.5.	Returning to on-line mode:.....	23

1. Safety

To safely operate or maintain this analyzer, all instructions in this manual must be read and fully understood by a trained/qualified technician.

Failure to follow safety procedures could result in serious injury or equipment damage.

The following symbols will be observed throughout this manual.



Protective Eye wear



Safety Gloves



Electrical Shock Hazard



Corrosive Hazard



UV Radiation Inside
Rayonnement ultraviolet à l'intérieur

2. ChemScan UV-Series Analyzer Description

The ChemScan UV-Series Analyzer is an on-line process-monitoring instrument. It has the capability of measuring multiple parameters in a sample. The precise measurement of these parameters is critical for optimizing today's advanced water treatment processes. It has been designed to minimize maintenance time and reagent costs.

The analyzer has a built-in manifold to accept samples from multiple locations. The analyzer is equipped with automatic zeroing and cleaning capability. Periodically the analyzer will pump zeroing solution into the flow cell. The analyzer tests for the need for cleaning the flowcell and zero stability. Once the diagnostic parameter is satisfied, the analyzer will return to the on-line sequence. If any abnormal operation is detected, the analyzer will alert the operator by displaying a "Maintenance Required" message.

2.1. Analyzer Analysis Modes

2.1.1. Flush Cycle

To begin the analysis the analyzer uses the new sample to flush the previous sample.

2.1.2. Scanning Sample

The analyzer flashes the xenon flash lamp that produces ultraviolet and visible light passing through the sample and detected in the spectrometer.

2.1.3. Reagent Addition

When reagent assisted analysis is required, the analyzer adds reagent to the sample cell.

2.1.4. Mixing Sample

The Analyzer uses air pumped through the cell to mix the sample

2.1.5. Idle or Reacting

The Analyzer is idle during the chemical reaction in the cell.

3. Operation


3.1. HMI Definition

3.1.1. HMI Components


Hardware Definition

3.2. Home Screen

The ChemScan Graphical User Interface provides access to analyzers operation, settings, diagnostics and help.

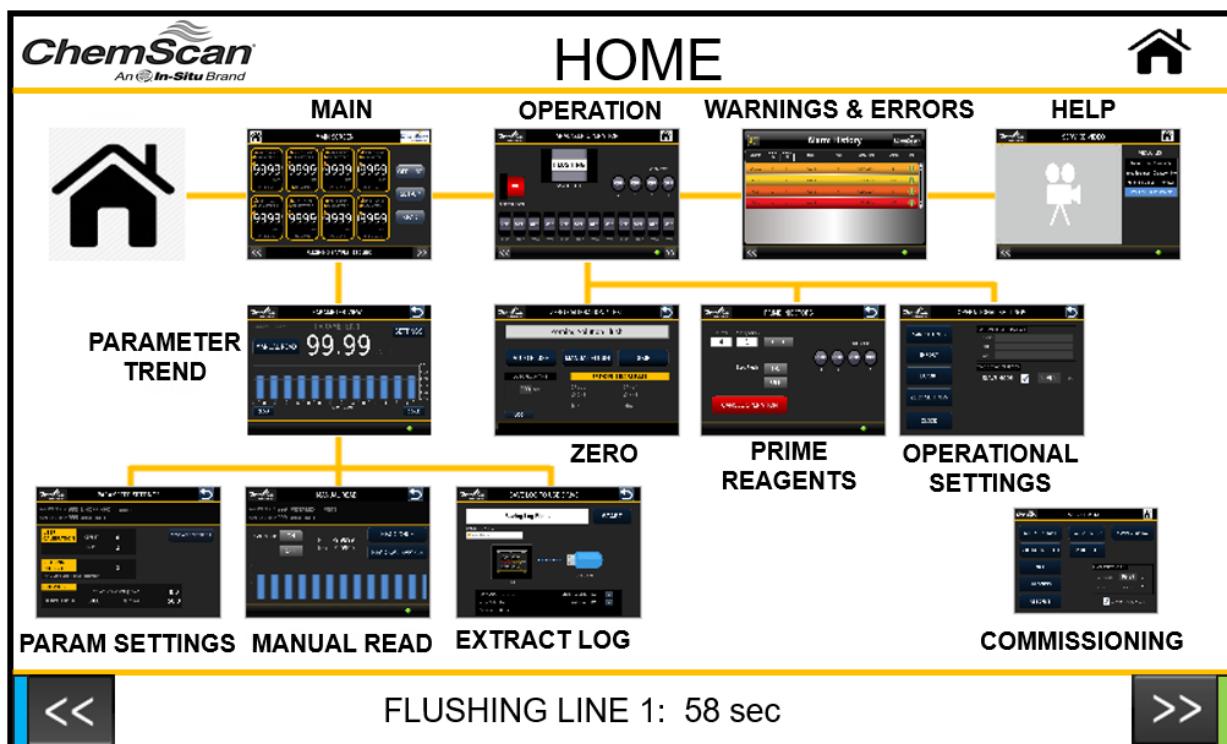

3.2.1. Home Screen – Top Level Buttons

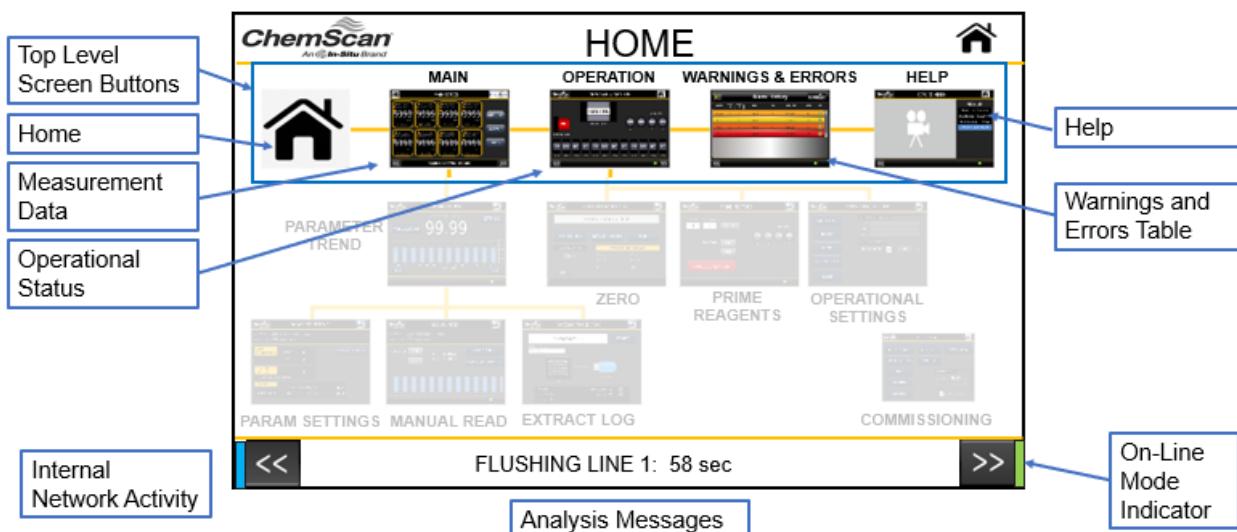

Home

This screen displays the overall HMI menu structure. *Tip: Press the ChemScan Log from any screen to return to the Home Screen.*

Measurement Data

Displays the most recent concentration data

Operational Status

Displays the Analyzer lower-enclosure operation and current analysis status

Warnings and Errors Screen

The warnings and errors screen contain analyzer operational malfunction data.

Help Screen

General Help Screen with access to the O&M Manual and demonstration videos.

Commissioning Screens

Accessible by ChemScan Technicians during startup and servicing the analyzer.

Analysis Message


The analyzer operational steps are displayed. These messages are similar to the legacy ChemScan products LCD display. *Tip: This is also a button to access the interrupt On-Line Mode from any screen.*

Indicator Lights

Internal Network Activity: This green light flashes during analyzer internal network activity.

On-Line Indicator: This is color red when Analyzer is in the On-Line continuous operation mode.

3.2.2. Home Screen – Parameter and Operation Groups

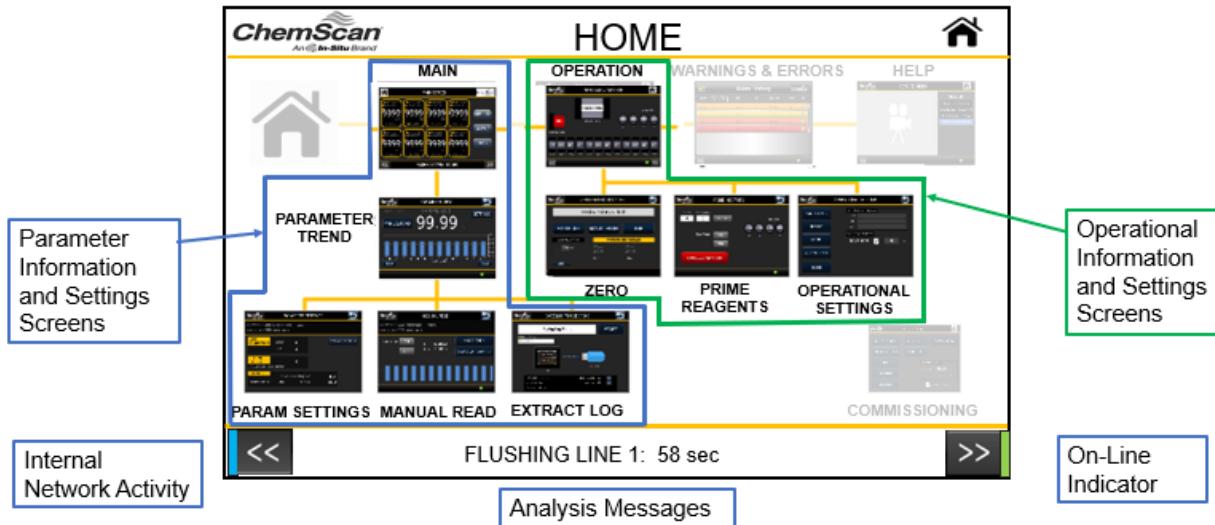


Parameter Information and Settings Screens

The items surrounded by the blue outline above, contain parameter concentration values, concentration trend, parameter settings, manual readings and concentration log retrieval.


Analyzer Operation Information and Settings Screens

The items surrounded by the green outline above, contain overall analyzer operational status, analyzer zero, prime reagents and operational settings.

3.3. Main Screen

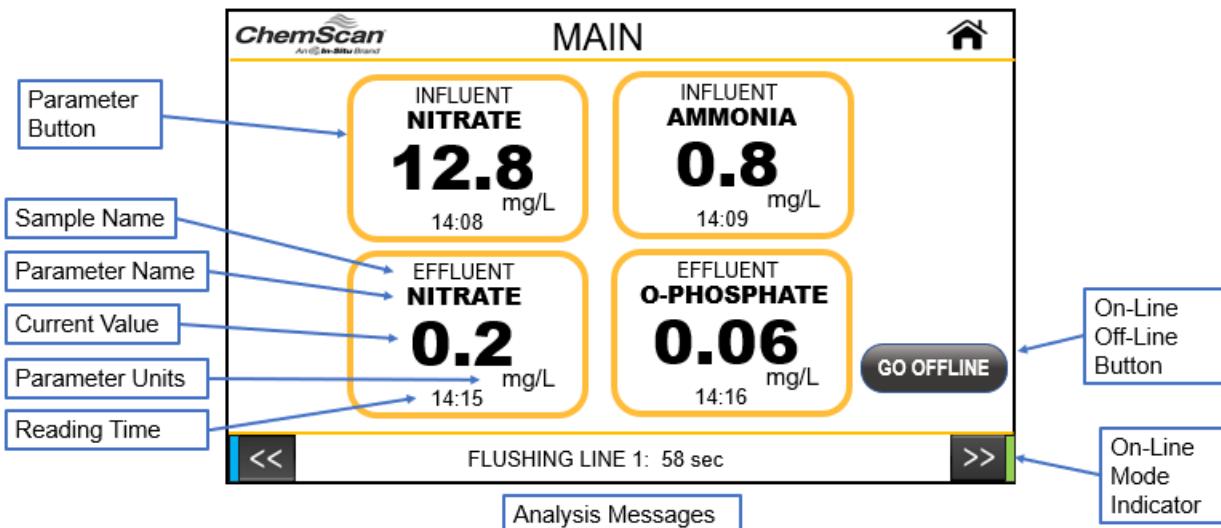


3.3.1. Initiate On-Line Mode

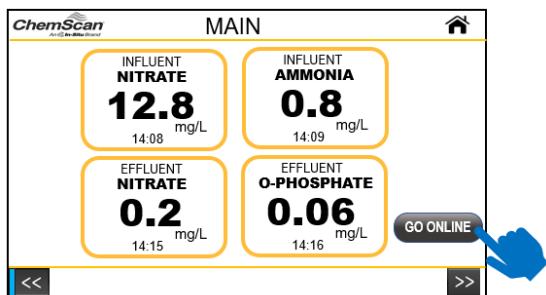


To enter the on-line mode, press the GO ONLINE button.

The Analyzer will begin the reading cycle at the first parameter on the first sample line.

3.3.2. Exit On-Line Mode

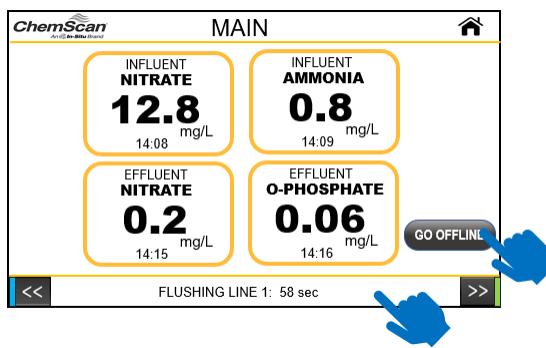


To exit the on-line mode, press the GO OFFLINE Button **OR** in **any** screen press the Analysis Message Bar at the bottom.

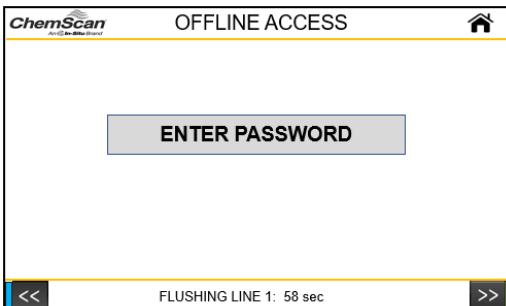

Then, enter the operator's level Password - Default Password: 0000

3.3.3. Navigation Short Cuts

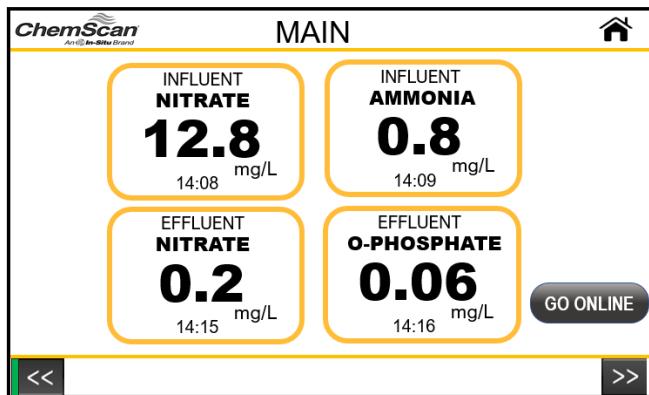

There are a few navigation tips to make it easier to move around the screens.

The top Left Corner **ChemScan** Logo button will return to the HOME Screen from any screen.

The Top Right Corner button will return back from the previous Screen.

In the on-line mode, the bottom **Analysis Message Bar** button will call up the security code to exit the on-line mode from any screen displaying the Analysis Information.

The bottle left arrows and right arrows will move across the Top Level Screens.

3.3.4. Parameter Screen Group


The parameter screen group is entered from the Main Screen by selecting one of the parameter buttons.



3.3.4.1. Parameter View Screen (On-Line Mode)


The Parameter View screen displays the currently selected parameters name, units, sample name, concentration, and a graph of the last 30 hours of operation. The Y scale can be changed using the +/- buttons in the lower right corner of the trend.

While the Diagnostics data can be displayed, the Parameter Settings can be displayed but not changed, and the Data Concentration Log can be extracted.

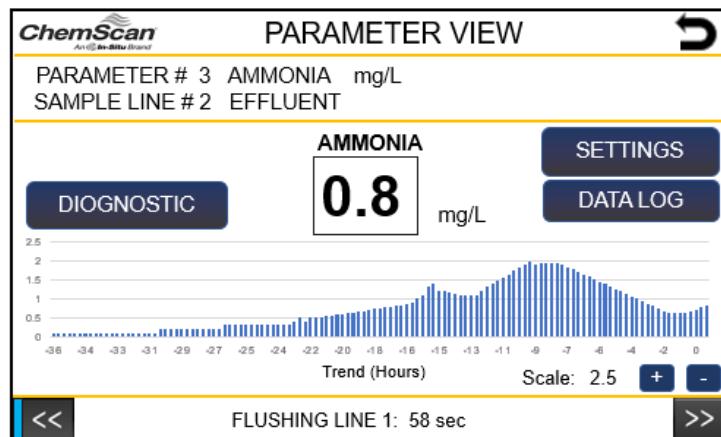

3.3.4.2. Parameter View Screen (Off-Line Mode)

While in the Off-Line Mode, the Manual Read is also displayed enabled. The Diagnostics data can be displayed, the Settings can be displayed and changed, and the Data Concentration Log can be extracted.

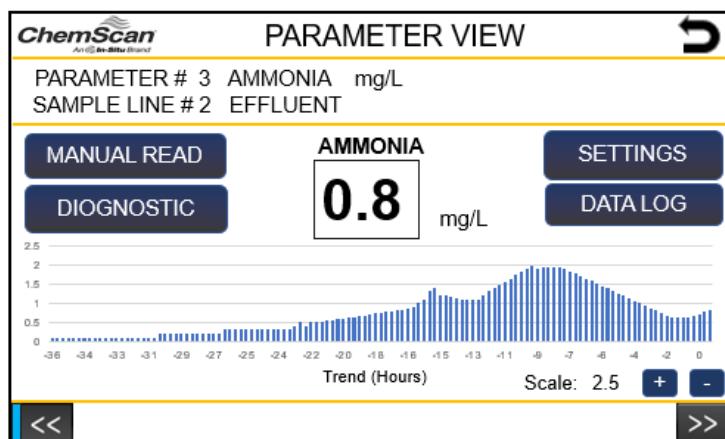

3.3.4.3. Parameter Settings Screen (Off-Line Mode)

PARAMETER SETTINGS

PARAMETER # 3 AMMONIA mg/L
SAMPLE LINE # 2 EFFLUENT

USER CALIBRATION OFFSET:
 SLOPE:

READING INTERVAL
NOTE: Set to Zero to disable parameter

OUTPUTS CONCENTRATION @ 4 mA:
ALARM SETPOINT: @ 20 mA:

<< >>

This screen allows users to set parameters for ammonia measurement. It includes fields for User Calibration (Offset and Slope), Reading Interval (set to 1), and Alarm Setpoint (0 mA). It also shows concentration values at 4 mA and 20 mA.

Calibration Offset: Adjust the parameter offset value.

Calibration Slope: Adjust the parameters slope value.

Reading Interval: Adjust the parameters reading interval, 1 = measure every cycle, 4 = measure every 4th cycle, 0 = Disable parameter.


Alarm Setpoint: Adjust alarm concentration value. Alarm active above the set concentration (dry contact relay or bit when serial is used) 0 = inactive.

4 mA Concentration: Adjust parameters 4 mA concentration when analog outputs are used. Default = 0.

20 mA Concentration: Adjust parameters 20 mA concentration when analog outputs are used. Default = max of parameters operating range.

The ADVANCED SETTINGS button requires a Technician level password. Contact ChemScan Service before making any adjustments in the advanced settings screen.

3.3.4.4. Parameter Manual Read Screen (Off-Line Mode)

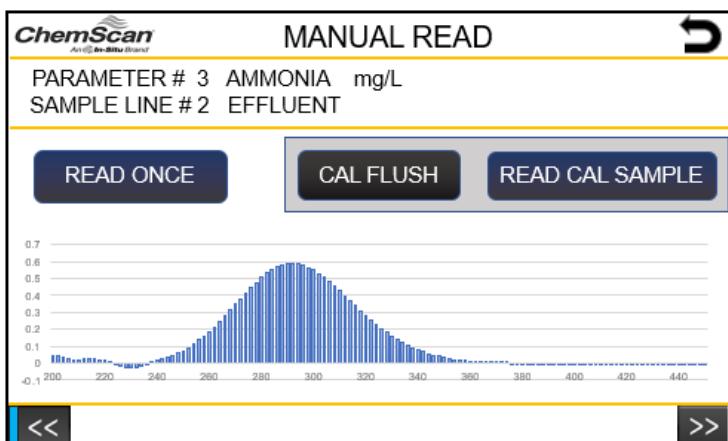


READ ONCE: The READ ONCE button initiates a single read of the selected parameter.

READ CAL SAMPLE: READ CAL Sample Button initiates a single reading of the sample currently in the analyzer's flow cell. Typically a calibration sample.

CAL FLUSH: Use the CAL FLUSH button to draw in a sample from the analyzer's calibration port into the cell prior to reading a calibration sample. Flush a minimum of 500 mL through the cell prior to initiating a READ CAL SAMPLE.

The previous sample's spectral data is displayed in the graph. This can be used to assist ChemScan Service while troubleshooting the analyzer.


3.3.4.5. Data log Retrieval Screen

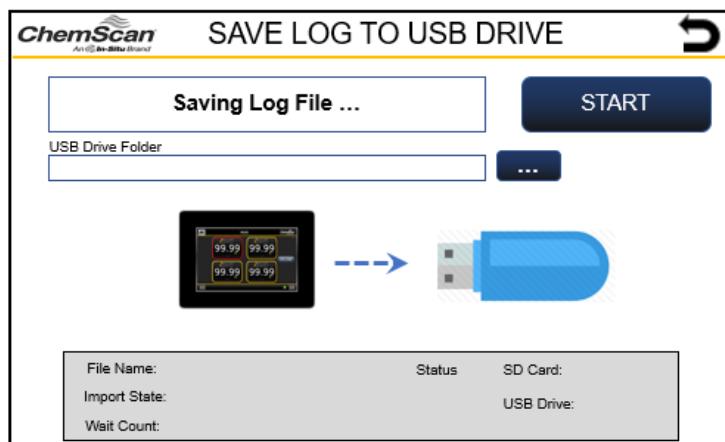


The analyzer's Concentration Data Log can be extracted to an USB drive by pressing the START button.

3.4. Operational Screen

Analyzer Operational Grouping

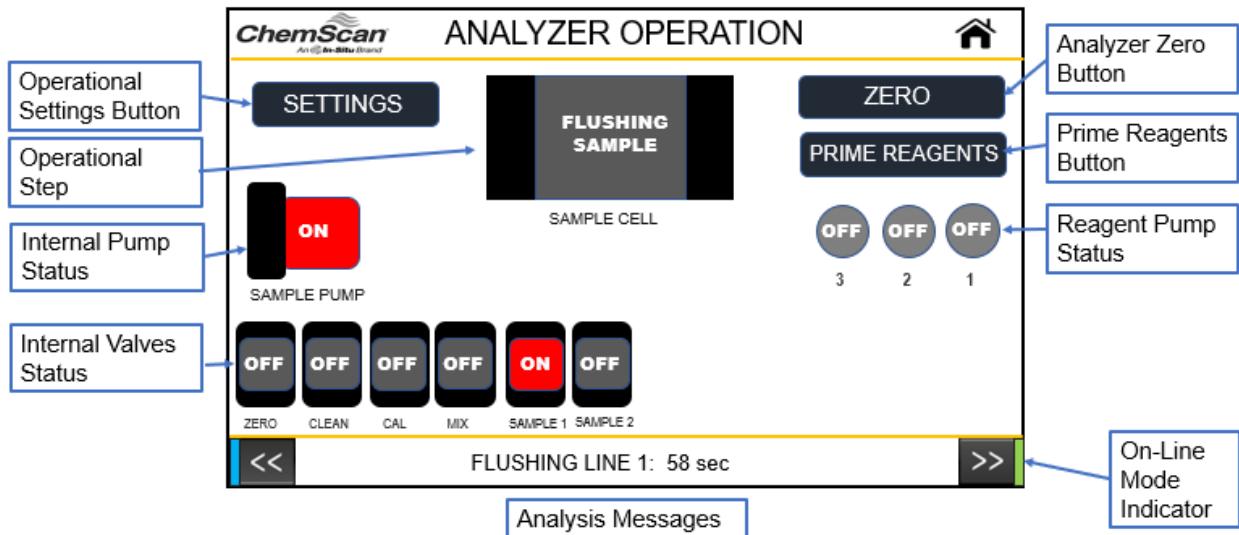


3.4.1. Analyzer Function Screen (On-Line Mode)

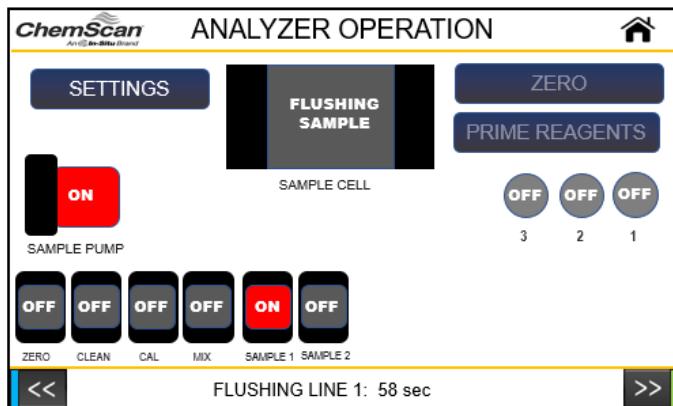

While in On-Line Mode the Analyzer Operation Screen will display status of the components during the analysis cycle. The Analyzer's operational SETTINGS Screen can be displayed but the edit function is disabled. The ZERO and PRIME REAGENTS buttons are disabled. Exit the On-line Mode to enable the ZERO and PRIME REAGENTS buttons and allow editing of the operational SETTINGS.

3.4.2. Analyzer Function Screen (Off-Line Mode)

While in Off-Line Mode the Analyzer Operation Screen the Analyzer's operational SETTINGS Screen can be displayed and edited. The ZERO and PRIME REAGENTS buttons are enable to access those functions.

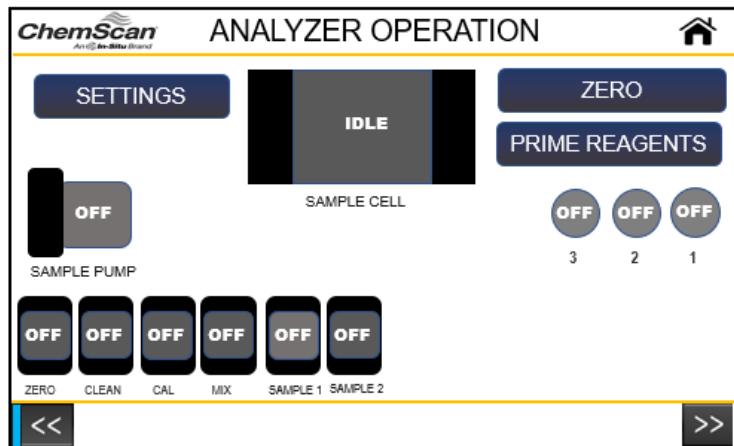


3.4.3. Manual Component Operation

While in the Off-Line Mode the Analyzer Operational Screen can be used to manually operate each component. This can be used during troubleshooting the analyzer.

To manually operate the component, press the component graphic. If the component requires a companion component to operate, both will turn on. (i.e. select the zero valve and the pump will operate too)


3.4.4. Analyzer Operation Group

The overall Analyzer's operation and settings is accessed through the buttons on the Analyzer Operation Screen.

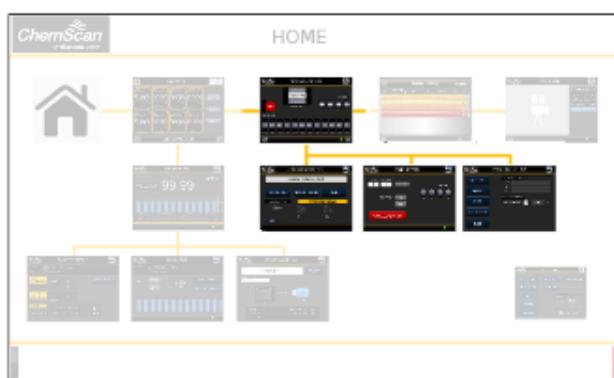


3.4.4.1. Manual Zero Screen

The Manual Zero Screen is used to perform the analyzer zeroing process. The Zero is the way to create an analyzer reference of the zero-absorbance water. This is also one of the main diagnostic tests to confirm the light level through the analysis cell. *See Manual Zero Operation in the Maintenance section.*

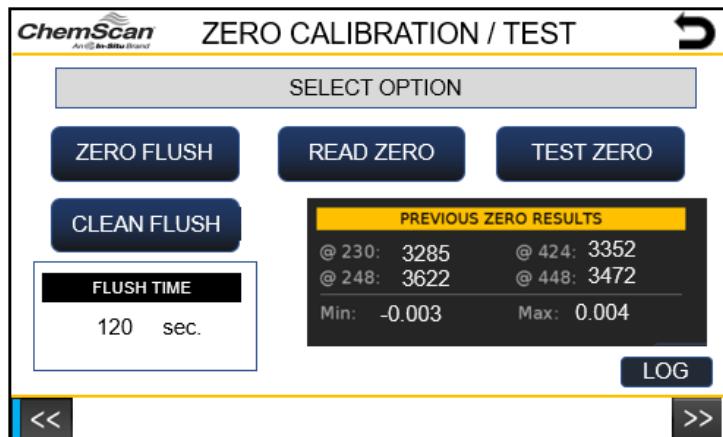


3.4.4.2. Prime Injectors Screen

The Prime Injector Screen is used to manually operate the reagent injector pumps to remove air from the reagent lines or test the reagent injector pump operation. *See Prime and Test Reagents Injectors in the Maintenance section.*

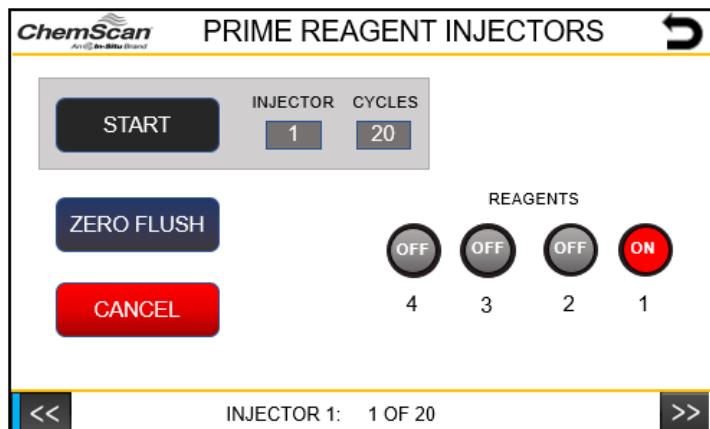

3.4.4.3. Operational Settings

The Operational Settings Screen provides access to the analyzer's overall operational configuration.

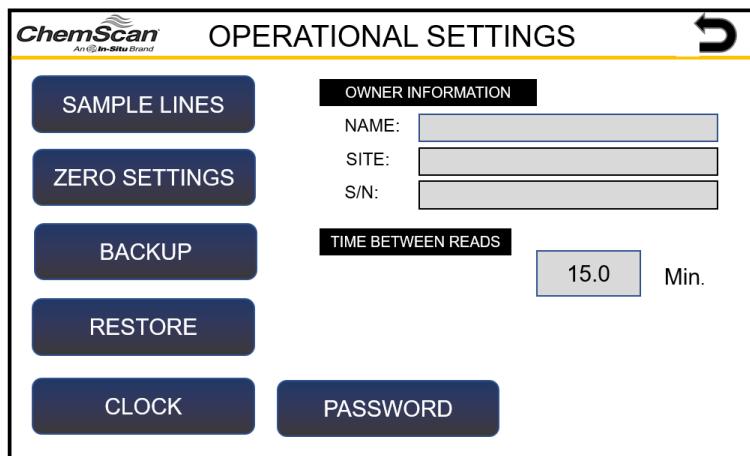

The Operational Settings screen for ChemScan. It features a sidebar with buttons for SAMPLE LINES, ZERO SETTINGS, BACKUP, RESTORE, CLOCK, and PASSWORD. The main area has sections for OWNER INFORMATION (NAME, SITE, S/N) and TIME BETWEEN READS (set to 15.0 Min.).


Installation Information:

Name: Organization or Company Name

Site: Plant or installation Name

S/N: Analyzer Serial Number

3.4.4.4. Sample Line Settings

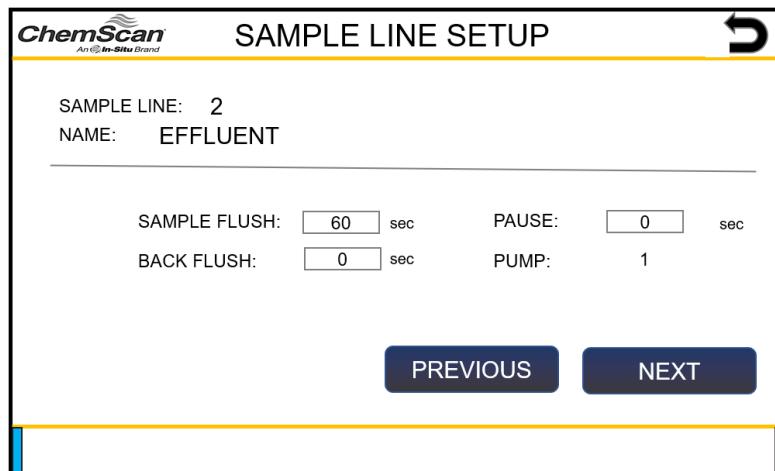

The Sample Line Setup screen for ChemScan. It shows a current sample line setup for Sample Line 2, named EFFLUENT. It includes fields for SAMPLE FLUSH (60 sec), PAUSE (0 sec), BACK FLUSH (0 sec), and PUMP (1). Navigation buttons PREVIOUS and NEXT are at the bottom.

Sample Line: Current Sample Line Number

Name: Sample Line Name

Sample Flush: Flush time before analysis

Back Flush: Time reverse flow (when a peristaltic pump), air blow back for certain filter systems with compressed air.

Pause Time: Setting time for some filter types.

Pump Number: Type of pump installed at the factory.

PREVIOUS/NEXT Buttons: Navigate between sample lines.

3.4.4.5. Zero Settings

The screenshot shows the 'AUTO ZERO/CLEAN SETUP' menu from the ChemScan UV-Series Analyzers Graphic User Interface. The menu includes settings for Auto Zero/Clean Interval, Auto Zero parameters (Installed), Auto Clean parameters (Installed), and Quick Clean parameters. It also displays Absorbance Limits and limits in A/D Counts. The 'Auto Zero/Clean Interval' is set to 48. Under 'Installed' Auto Zero, the 'Flush Time' is 90 sec and 'Test Flush Time' is 20 sec. Under 'Installed' Auto Clean, the 'Flush Time' is 40 sec and 'Pause Time' is 120 sec. Under 'QUICK CLEAN', the 'Flush Time' is 20 sec and 'Interval' is 24. Absorbance limits are set to Max: 0.01 and Min: 0.01. Limits in A/D Counts are @230: 1500, @424: 100, @248: 1500, and @448: 100.

Auto Zero/Clean Interval: Number of cycles between Zero/Clean cycles

Quick Clean Interval: Number of cycles between Quick Clean cycles

Quick Clean Flush Time: Time to flush cleaning solution during a quick clean.

Quick Clean Rinse Time: Time to rinse sample after a quick clean.

All other parameters require contact with ChemScan Service prior to adjusting.

3.4.4.6. Memory Backup

The screenshot shows the 'CONFIGURATION BACKUP' menu from the ChemScan UV-Series Analyzers Graphic User Interface. The menu title is 'CONFIGURATION BACKUP' and it displays 'BACKUP ANALYZER'S CONFIGURATION'. A large blue 'BACKUP' button is centered on the screen.

- 1) The BACKUP button will store the current configuration savings to the internal SD memory card.
- 2) A second step will allow backup to a USB drive.


3.4.4.7. Memory Restore



SD CARD button will restore the configuration stored on the internal SD card.


USB DRIVE button will restore the configuration stored on the external USB Drive.

3.4.4.8. Clock and Screen Settings

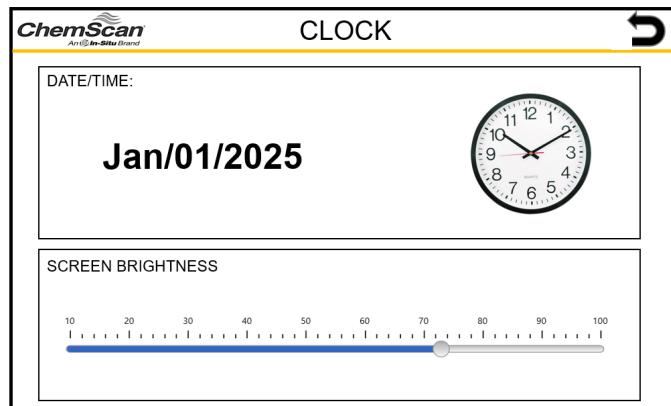


Set the clock and screen intensity.

3.4.4.9. Password Settings

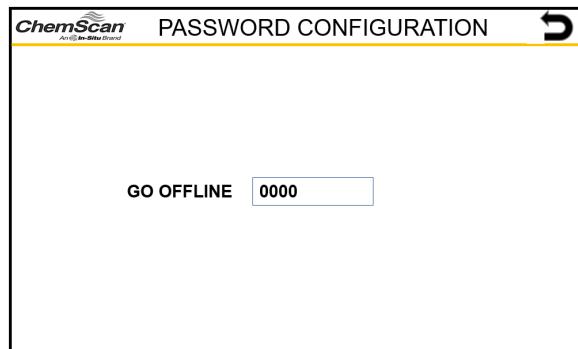


Set the security code to interrupt the On-Line mode.

3.4.5. Warnings and Errors –

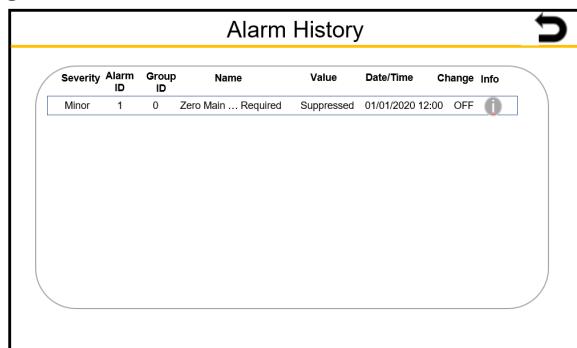

Displays the internal operational warnings and alarms.

3.4.6. Help

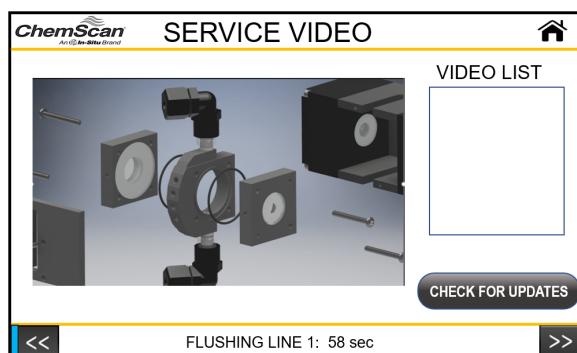

Displays videos and animations of critical service items.

4. Maintenance

4.1. Manual Analyzer Zeroing Procedure


The ChemScan UV-Series Analyzer must be zeroed occasionally to correct for drift and flow cell fouling. The analyzer will automatically perform a zero on a regular basis (typically daily).

However it is important to periodically perform a Manual Zero Operation to track the indicator numbers. This procedure simply involves rinsing the flow cell with deionized water, initiating a zero reading and testing the zero.

Items Required:

1 gallon of deionized water


4.1.1. Interrupt on-line mode:

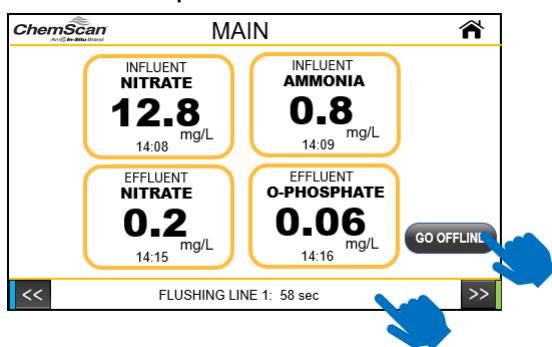


To exit the on-line mode, press the GO OFFLINE Button **OR** in **any** screen press the Analysis Message Bar at the bottom.

4.1.2. Analyzer Operation Screen

Navigate to the ANALYZER OPERATION screen, then press the ZERO button.

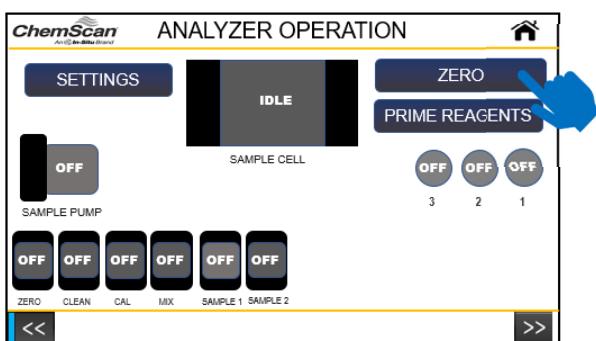


4.1.3. Analyzer Zero Screen – Reading the Zero

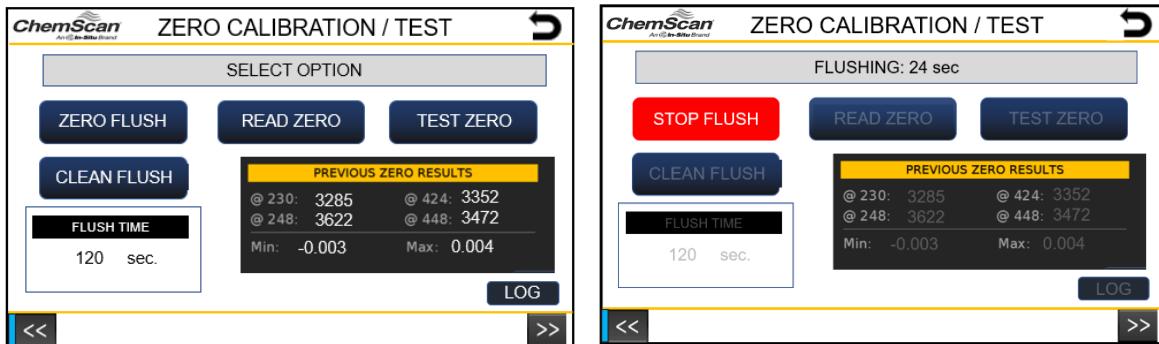

Press the ZERO FLUSH button to begin flushing the deionized water. Allow the water to flush for 2 minutes and press STOP FLUSH to stop flushing. Allow the water to settle in the flowcell for 10 – 15 seconds.

Press READ ZERO button to Read and store the zero-absorbance water.

4.1.4. Analyzer Zero Screen – Testing the Zero

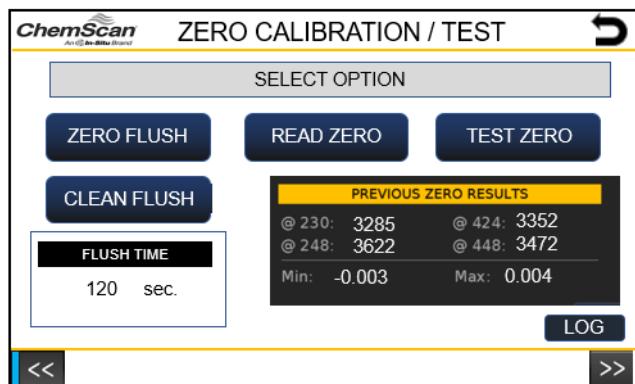


Press the ZERO FLUSH button to begin flushing the deionized water. Allow the water to flush for 15 – 20 seconds and press STOP FLUSH to stop flushing. Allow the water to settle in the flowcell for 10 – 15 seconds.

Press TEST ZERO button to Read and store the zero-absorbance water. The “Previous Zero Results” will update when the Test Zero reading is finished.

If the MX value is greater than 0.005 or if the MN value is less than -0.005 repeat the Zeroing procedure. If the 230 or 248 values are less than 2500, the flow cell should be chemically cleaned.

4.1.5. Returning to on-line mode:

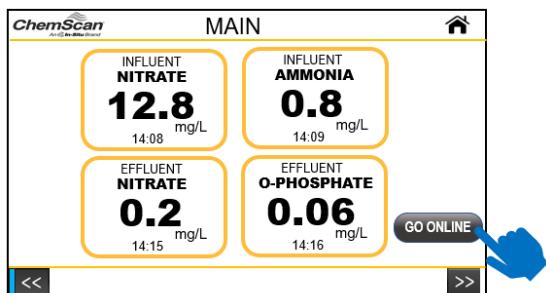

www.in-situ.com

1-800-446-7488 (toll-free in U.S.A. and Canada) • 1-970-498-1500 (U.S.A. and international)

221 East Lincoln Avenue, Fort Collins, CO 80524 USA

Copyright © 2022 In-Situ Inc. All rights reserved. January 2022